ticare TISSUE CARE PHILOSOPHY

DRILLING SEQUENCE

Ticare Osseous

STANDARD SEQUENCE

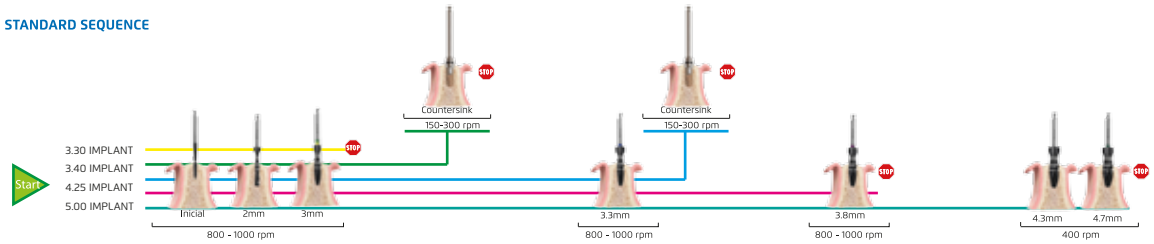

HARD BONE SEQUENCE

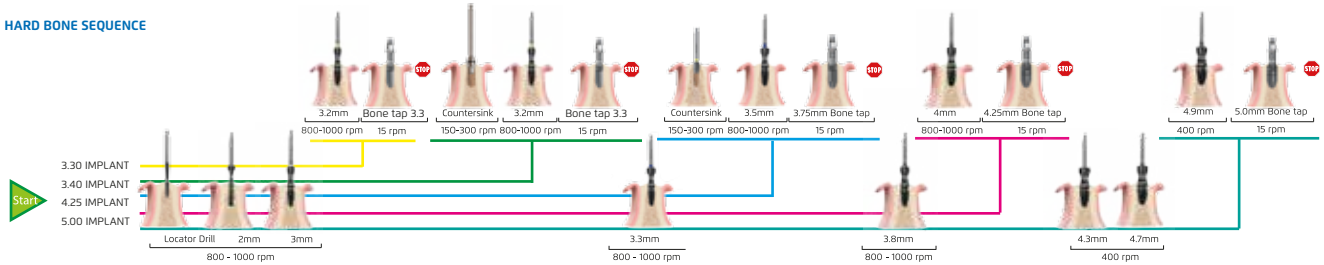

Ticare Inhex

STANDARD DRILLING SEQUENCE

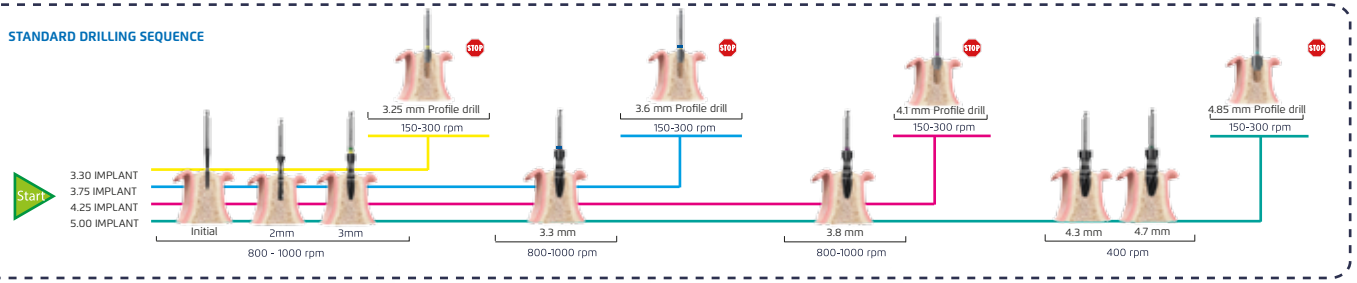

HARD BONE SEQUENCE

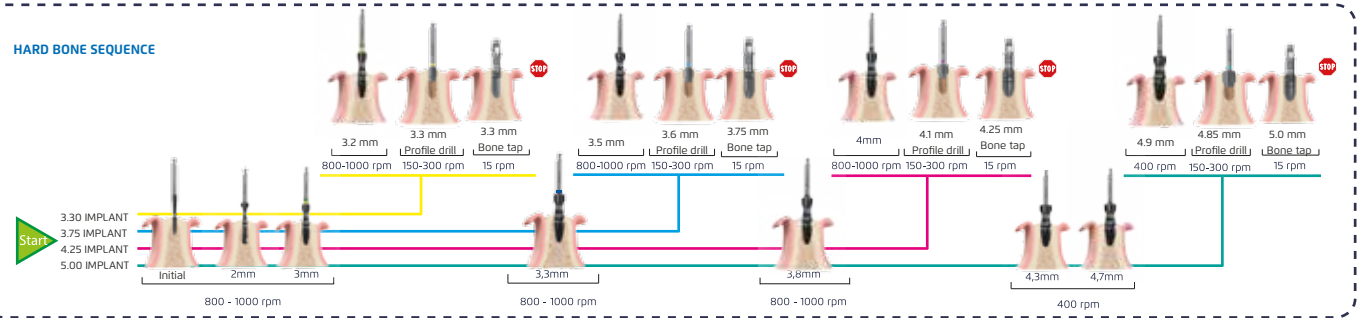

Profile drills should not be used for 6 mm long implants

Ticare Osseous Quattro

STANDARD SEQUENCE BONES TYPE III AND IV

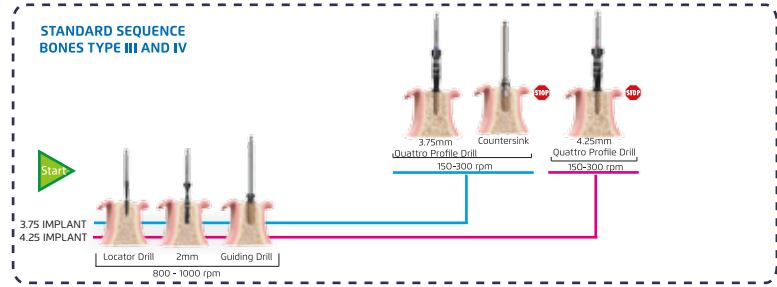

BONES TYPE II SEQUENCE

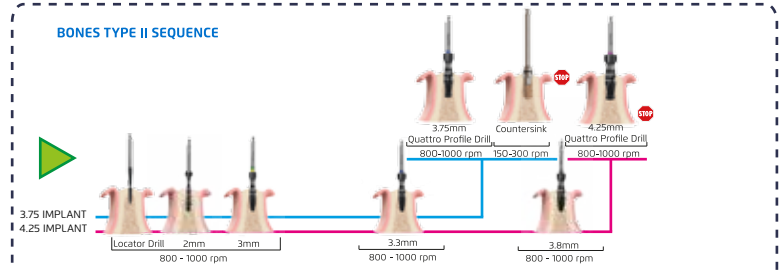

Quattro implants are not recommended for bone type I

Ticare Inhex Quattro

STANDARD SEQUENCE BONES TYPE III AND IV

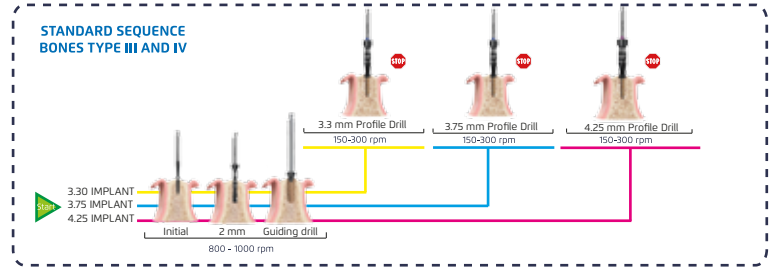

BONES TYPE II SEQUENCE

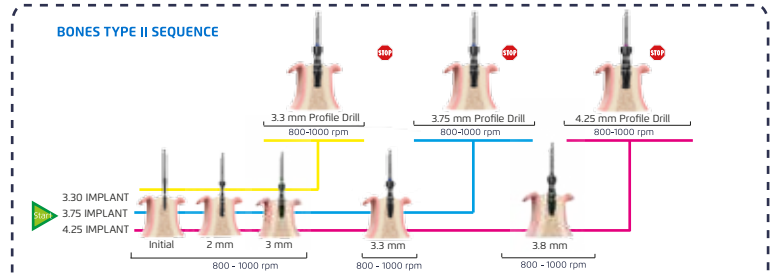

Quattro implants are not recommended for bone type I